

SILENCER®

S2410SP Series

Instruction Manual



Proudly designed and manufactured in the great United States

Copyright © 2019

Global Focus Marketing & Distribution, Ltd.

2280 Springlake # 106

Dallas, Texas 75234

800-323-4306

<https://gfmd.com/support/>

This manual contains confidential and proprietary information, and is provided to Silencer[®] customers under license. Receipt of this manual does not convey any rights to reproduce or disclose its contents in any form. Global Focus Marketing & Distribution, Ltd. (herein known as GFMD, Ltd) retains all rights to this manual and its contents. Reproducing and/or disclosure of its contents is strictly prohibited, and may violate Copyright and/or Patent laws.

While every effort has been made to ensure the completeness and accuracy of this manual, Global Focus Marketing & Distribution, Ltd. will not be liable for failure to follow standard safety precautions.

Printed in the United States of America.

Table Of Contents

Chapter 1	Getting Started	1-1
	Scope	1-1
	Unpacking And Inspection.....	1-1
	Setup.....	1-1
	Rotor Installation	1-2
Chapter 2	About The S2410SP.....	2-1
	Purpose	2-1
	Description	2-1
Chapter 3	Using The S2410SP	3-1
	Orientation.....	3-1
	Controls	3-1
	Operation	3-2
	Set Point	3-2
	Program Store	3-3
	Program Recall	3-3
	Settings Menu	3-4
	Operation Tips	3-5
	Operation Flowchart	3-6
Chapter 4	Cleaning	4-1
Chapter 5	Troubleshooting	5-1
	Status Codes	5-1
	Error Reset.....	5-1
	Troubleshooting Table	5-1
Chapter 6	Warranty	6-1
Appendix A	Specifications	A-1
	Performance Specifications.....	A-1
	Unit Specifications.....	A-2
Appendix B	R. C. F. Chart	A-3
Appendix C	Service Log	A-5
Appendix D	Replacement Parts List	A-6
Appendix E	Lid Release Tool.....	A-7

Chapter 1

Getting Started

SCOPE

This manual contains information with regards to application, installation, and operation of the Silencer[®] S2410SP benchtop centrifuge, and must be read prior to setup or operation of the centrifuge.

UNPACKING AND INSPECTION

Your new Silencer[®] centrifuge is packed in a specially designed shipping carton. Upon arrival please check the condition of carton and note any damage. Keep all packing materials for the warranty period of the centrifuge.

After unpacking your Silencer[®] carefully inspect it for damage. It is your responsibility to report all damages to the transportation company and filing, if necessary, any damage claims.

At this point take a moment to ensure you have received the correct rotor, tube adapters, etc. If not or if you have any questions regarding compatibility with your tubes, please contact GFMD, Ltd. at 800-323-4306 before proceeding.



WARNING

Do not operate this equipment in a combustible atmosphere!

SETUP

For your own safety and to prevent damage to the centrifuge, be sure to read this manual before continuing with setup or operation of this centrifuge.

For smooth operation and long equipment life, choose a stable, level bench top.

Avoid sources of heat and/or moisture such as sinks, water baths, heating ducts, and direct sunlight. A suitable environment is 10° to 30° C (50° to 86° F) with a relative humidity range of 40% to 70%. The minimum clearance is 6" on all sides. A cooler ventilated location and leaving the lid open between cycles will allow longer and/or more frequent cycles without overheating of samples. The maximum number of cycles that may be run consecutively will depend upon operating speed, set time, ventilation around the centrifuge, and ambient temperature. Samples that may be adversely affected by being warmed to 39°C during centrifugation should be centrifuged in a refrigerated centrifuge such as the Silencer[®] S2510R.

Plug the power cord into a properly grounded outlet and turn on main power interrupt (on back of unit next to power cord). For safety, equipment life, and proper performance, your Silencer[®] S2410SP's power requirements are 115V AC, 5 amperes, 60Hz. The power cord must be UL listed or CSA certified, 18 AWG, and 6' 7" or less in length.

Getting Started

WARNING

Operating the centrifuge without proper grounding can cause dangerous electrical conditions and could result in serious operator injury!

CAUTION

Operation of centrifuge on an emergency power circuit can cause damage to electronic circuits.

CAUTION

Operation of centrifuge on a power strip increases ground resistance and can cause damage to electronic circuits.

ROTOR INSTALLATION

Insert the rotor onto the motor shaft ensuring the alignment pin in the motor shaft fits correctly into the alignment groove in the bottom of the rotor. The rotor must be installed correctly for proper operation.

Replace the rotor securing nut. The nut must be securely tightened.

About The S2410SP

PURPOSE

The Silencer[®] S2410SP is a quiet, general purpose centrifuge designed to be used to accelerate sample separation through the application of relative centrifugal force (RCF). This product is not intended to diagnose, treat, cure or prevent any disease.

DESCRIPTION

The direct drive system employs a powerful, specially designed, balanced, brushless motor ensuring a smooth quiet operation spanning the full speed range of the instrument. This design also promotes long bearing life and eliminates brush maintenance, thereby reducing operating costs.

Excellent stability against imbalance is achieved due to special vibration absorbing drive assembly mounts.

The operator and the S2410SP are protected by several safety features:

- The centrifuge cannot be started with the lid open.
- The centrifuge will not run if the lidlock fails to securely lock.
- Once the rotor is in motion the lid cannot be opened until the rotor has stopped.
- The see-through high-strength lid allows the operator to view the rotor chamber without opening the lid.
- The rotor chamber is strong and easy to clean.

For complete equipment specifications see Appendix A.

Chapter 3

Using The S2410SP

ORIENTATION

Take time now to acquaint yourself with the S2410SP's displays and controls. The basic operation is very simple and the controls are mostly self-explanatory.

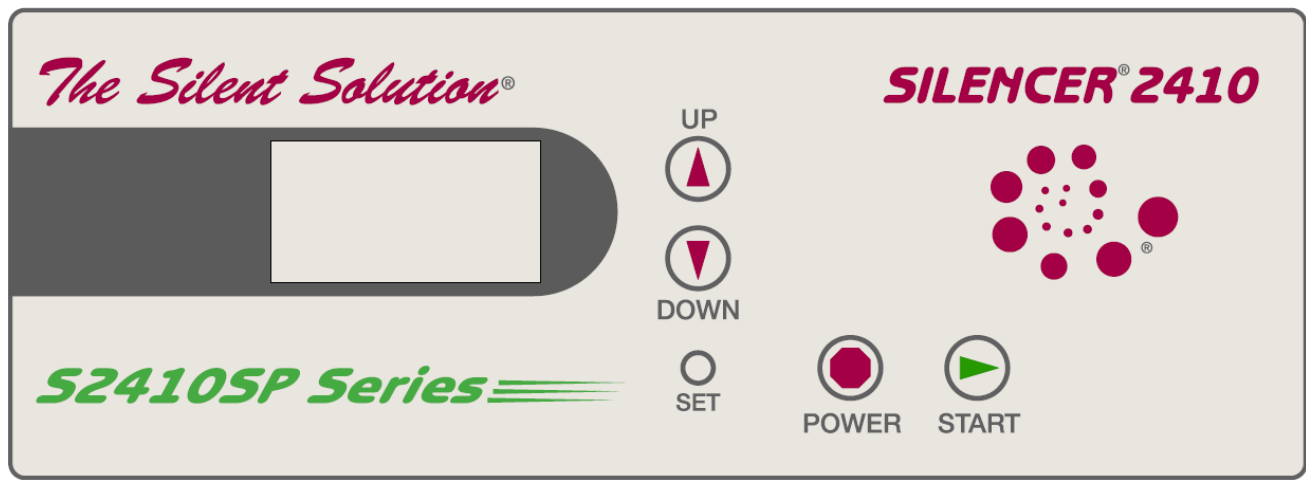


Figure 3.1



WARNING

Turning the power off does not remove power to the centrifuge. Remove all power to the unit by unplugging the power cord.

CONTROLS

POWER

Press the POWER button once to bring the unit out of SLEEP mode and into STANDBY mode. This unlocks the lid and turns the display on. Pressing the POWER button while the power is on turns the display off and puts the unit into a low power SLEEP mode.

Pressing the POWER button during a run cycle stops the cycle.

Pressing the POWER button while in any SET mode cancels and returns the centrifuge to the STANDBY MODE.

SET

Press to enter the SET POINT mode

UP

Press the UP button to increase the value of the selected item.

Using The S2410SP

DOWN

Press the DOWN button to decrease the value of the selected item.

START

If pressed when the unit is in the STANDBY mode, the START button will start the run cycle, which is indicated by the display going into inverse mode (dark background and light text).

Pressing the START button while in any SET mode will accept changes and return to the STANDBY mode.




WARNING

Do not operate this equipment in a combustible atmosphere!

OPERATION

Chapter 1 must be read and the S2410SP must be setup accordingly before continuing.

Press the POWER button to bring the centrifuge out of the SLEEP mode, turn the display on, and unlock the lid.

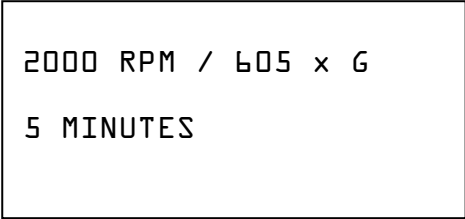

2000 RPM / 605 x G
5 MINUTES

The set speed and time defaults to the last saved speed and time setting. The settings can be changed in the SET POINT mode or a saved program can be recalled in the PROGRAM RECALL mode.

Open the lid and load your samples, taking care to maintain a balanced load.

Close the lid and press the START button. The lidlock will engage, the display will show the actual speed, and the centrifuge will accelerate to the set speed. Upon reaching the set speed the time will start counting down, and the display will show the time remaining.

When the set time has elapsed, the centrifuge will decelerate to a stop.

When the rotor has come to a complete stop the lidlock will release, and display will revert back to set speed and time.

SET POINT

The SET POINT mode shows the current speed and time settings.

NOTE: The current settings can not be changed if the centrifuge is in the LOCKED mode.

Using The S2410SP

```
SET POINTS
▶ RPM: 2000 RCF: 0605
  TIME: 005 MINUTES
```

The currently selected item is indicated with an arrow. To select another parameter for modification press and release the SET button.

Modify the selected parameter by pressing the UP or DOWN button.

Cancel changes by pressing the POWER button.

Accept the changes and return to the STANDBY mode by pressing the START button.

If you wish to save these settings press and hold the SET button for approximately two seconds to enter the PROGRAM STORE mode (indicated by three short beeps).

PROGRAM STORE

The PROGRAM STORE mode displays the three program locations.

```
PROGRAM - STORE
▶ PROG NUMBER: 1
  PROG NUMBER: 2
  PROG NUMBER: 3

RPM    TIME
2000   005
```

The currently selected program is indicated with an arrow. Press the SET button to select another program location.

The current saved speed and time for the selected program is displayed below the program list.

Press the POWER button to cancel programming and return to the STANDBY mode.

Press the START button to store the settings into the selected program location and return to the STANDBY mode.

PROGRAM RECALL

Press and hold the SET button for approximately 2 seconds to enter the PROGRAM RECALL mode (indicated by three short beeps).

The PROGRAM RECALL mode displays the three selectable programs.

Using The S2410SP

```
PROGRAM - RECALL
▶ PROG NUMBER: 1
  PROG NUMBER: 2
  PROG NUMBER: 3

RPM      TIME
2000     005
```

The currently selected program is indicated with an arrow. Press the SET button to select another program location.

The programmed speed and time for the selected program is displayed below the program list.

Press the POWER button to cancel program selection and return to the STANDBY mode.

Press the START button to accept the program selection and return to the STANDBY mode.

SETTINGS MENU

Press the POWER button to put the centrifuge into the SLEEP mode (indicated by one beep).

Press and hold the SET button while pressing and releasing the POWER button.

Continue to hold the SET button until the unit enters the SETTINGS MENU (indicated by 2 short beeps)

Release the SET button.

```
SETTINGS MENU
▶ BEEPS (EOR):      1
  BEEPS (error):    5
  RCF MODE:         OFF
  OPTIONAL EOR LED: 2
```

The SETTINGS MENU shows the current user settings.

The currently selected item is indicated with an arrow. To select another parameter for modification press and release the SET button.

Modify the selected parameter by pressing the UP or DOWN button.

Accept the changes and return to the STANDBY mode by pressing the START button.

BEEPS (EOR)

This determines the number of times the centrifuge will beep at the end of each run. The default is 1 and the allowable settings are 0 to 9.

Using The S2410SP

BEEPS (error)

This determines the number of times the centrifuge will beep when an error is incurred. The default is 5 and the allowable settings are 5 to 9.

RCF MODE

This allows the operator to choose how speed will be set. If the RCF MODE is OFF the speed is set by RPM in 100 RPM increments. If the RCF MODE is ON the speed is set by RCF in increments of 10xg.

OPTIONAL EOR LED

This setting has no effect unless the optional End of Run Light is installed. This setting determines the length of time (in minutes) that the green LED will remain on at the end of each run. The default is 2 and the allowable settings are 0 to 99.

OPERATION TIPS

- Do not drop or slam the lid!
- Use the emergency lid lock release only for emergencies.
- Only use the supplied emergency lid lock release tool.
- Unplug the centrifuge before using the emergency lid lock release tool.
- Leave the lid open between cycles.

If there are any questions regarding operation please contact GFMD, Ltd. at 800-323-4306.

Using The S2410SP

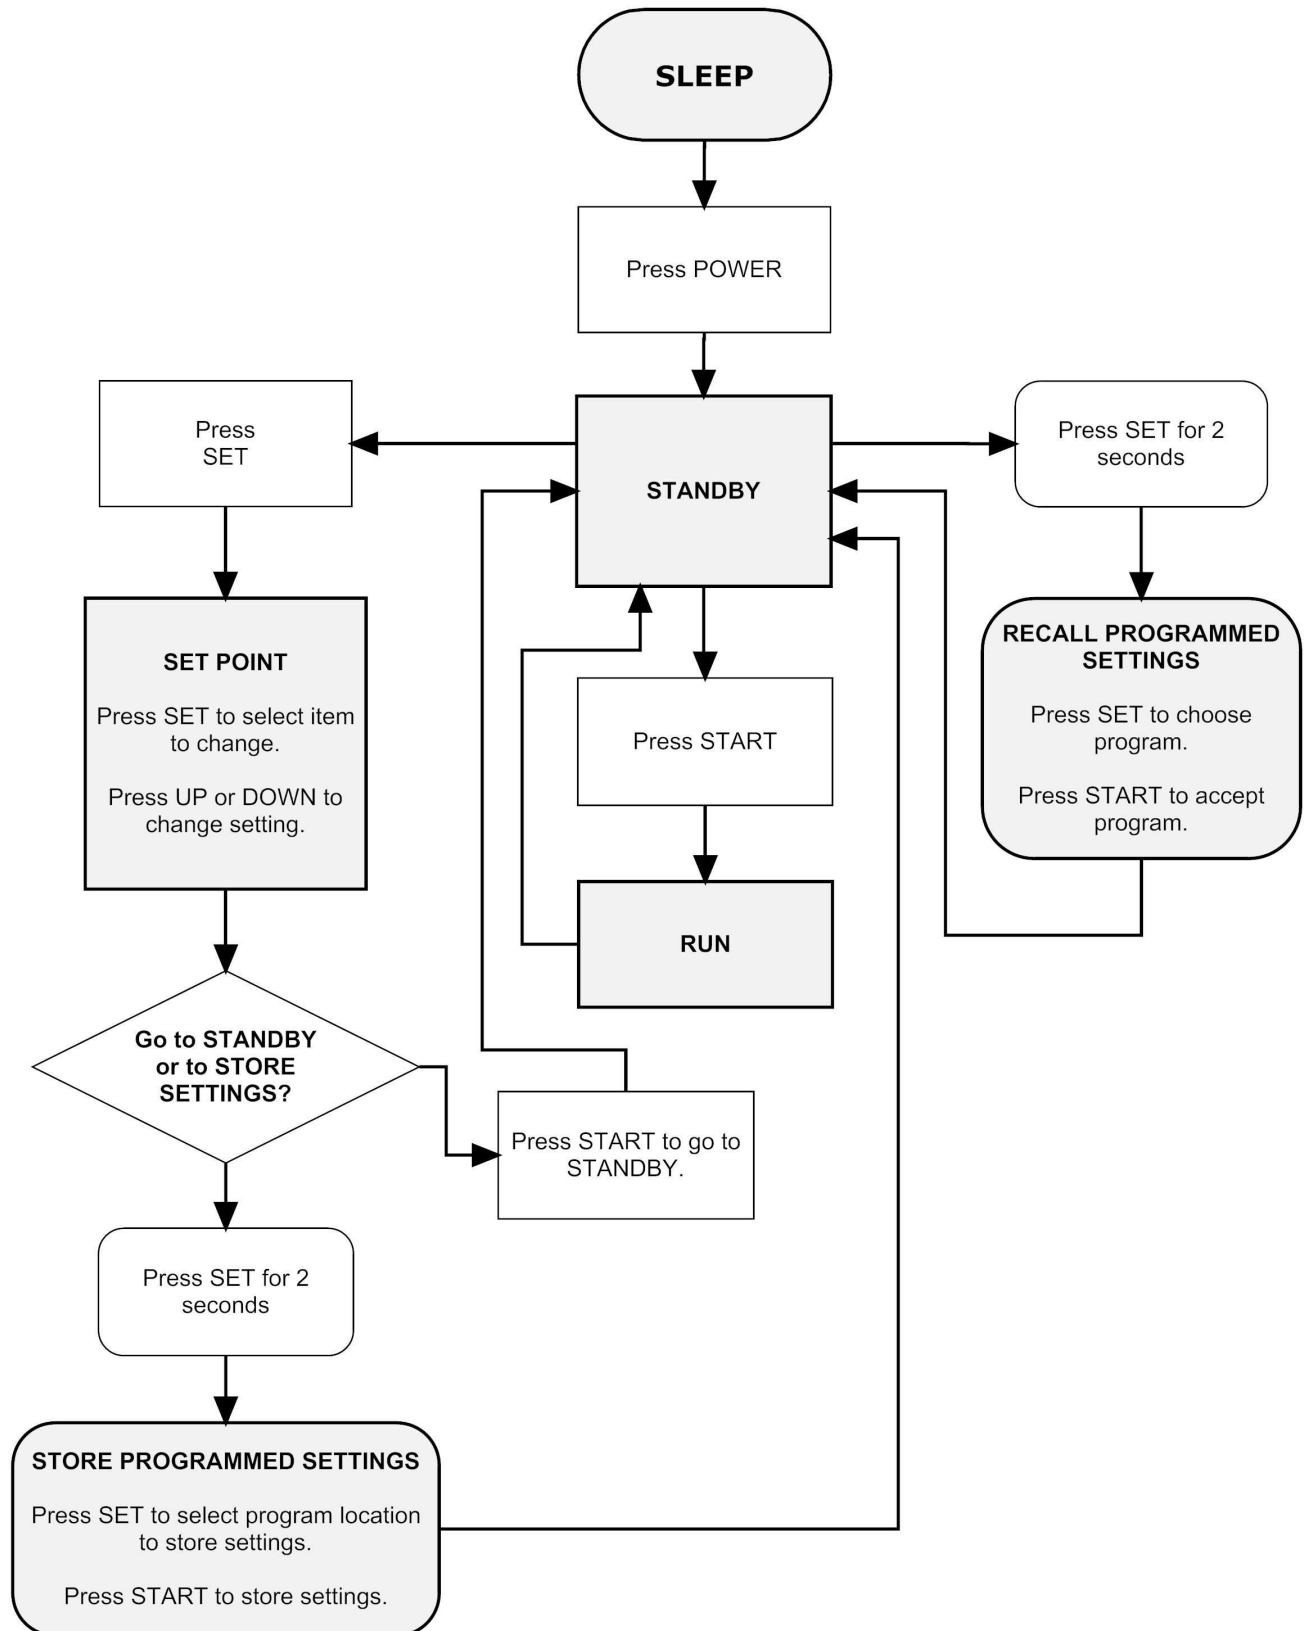


Figure 3.2

Cleaning

⚠ WARNING

Turning the power off does not remove power to the centrifuge. Remove all power to the unit by unplugging the power cord.

⚠ WARNING

Standard safety precautions for handling of biological hazards must be followed!

CAUTION

Do not get any liquids into the top of the motor. Many disinfectants are extremely corrosive and may damage the motor.

CAUTION

Allowing liquid levels in the rotor chamber to rise to the bottom of the motor seal may result in serious damage to the centrifuge.

- The rotor must be removed from the centrifuge for disinfecting.
- Clean tube breakages and spills immediately and thoroughly. The interior can be disinfected with disinfectants such as bleach, followed by a clear water rinse and wipe. The interior must be rinsed and dried thoroughly before using the centrifuge. Use water sparingly when rinsing, as the motor seal is not watertight.
- The exterior should be kept clean with the use of a mild soap and a damp (not wet) lint-free cloth. The centrifuge must be dried thoroughly before using.

Chapter 5

Troubleshooting

STATUS CODES

This is a list of error codes and the brief description that the centrifuge displays when an error is encountered. Check under symptoms for more details.

ERROR: 1.1	Indicates no power is getting to the motor.
ERROR: 1.2	Indicative of low line voltage or a momentary sag.
ERROR: 1.3	Indicative of a momentary drop or loss of line voltage. (LOCKING)
ERROR: 7.1	Check the lid safety interlock switch for proper alignment and continuity.
ERROR: 7.2	Check the lid safety interlock switch for proper alignment and continuity.
ERROR: 7.3	Do not attempt to open the lid until the unit has stopped. (LOCKING)
ERROR: 8	Ensure the line voltage is stable & the circuit isn't overloaded.

ERROR RESET

Pressing the front panel POWER button will reset most error messages.

Locking errors indicate an issue that needs to be addressed before the unit is put back into service. Unplug the centrifuge for approximately 20 seconds in order to reset locking errors.

TROUBLESHOOTING TABLE

SYMPTOM	The lid remains locked and the displays are not illuminated when the POWER button is pressed.	
	POSSIBLE CAUSES	POSSIBLE SOLUTIONS
	No power to the S2410SP.	Ensure the S2410SP is plugged in, there is power to the receptacle, and the main power switch is on.
	The fuses are blown.	Replace the fuses with 5A, 250V, time delay fuses. If the fuses blow again contact GFMD, Ltd. at 800-323-4306 for assistance.

Troubleshooting

SYMPTOM	Will not start when the START button is pressed and “ERROR: 7.1” is displayed.	
	POSSIBLE CAUSES	POSSIBLE SOLUTIONS
	The lid safety interlock switch is defective or misaligned.	Check the lid safety interlock switch for proper alignment and continuity.
	Lid is not closed completely preventing the lid from locking.	Make sure the lid is completely closed.
	Locking mechanism is mechanically binding.	Check for proper lid lock solenoid movement.
	Lid lock safety interlock switch is defective or misaligned.	Check the lid lock safety interlock switch for proper alignment and continuity.

SYMPTOM	Will not start when the START button is pressed and “ERROR: 1.1” is displayed.	
	POSSIBLE CAUSES	POSSIBLE SOLUTIONS
	Indicates no power is getting to motor.	Ensure the motor wires are properly connected to MOTA1, MOTB1, and MOTC1 on the Power PCB.
	The motor tachometer cable is unplugged.	Ensure the motor tachometer cable is connected to MOTOR1 on the Power PCB.
	The power sagged so the unit did not start before the bootstrap capacitors discharged.	Check electrical outlet for stable line voltage, and ensure that the circuit isn't overloaded. Reset the unit by turning the main power switch off for approximately 20 seconds and then back on.

Troubleshooting

SYMPTOM	Shuts down and a status code is displayed.	
	POSSIBLE CAUSES	POSSIBLE SOLUTIONS
	ERROR: 1.2 - Indicative of low line voltage or a momentary sag in line voltage.	Check for a loose power cord connection to the outlet, an overloaded circuit, or line voltage below 110 VAC.
	ERROR: 1.3 - Indicative of a momentary drop in line voltage or loss of line voltage.	Reset the unit by turning the main power switch off for approximately 20 seconds and then back on.
	ERROR: 7.2 - Indicates the lid safety interlock switch failed during a run cycle or an attempt was made to open the lid during the run cycle	<p>If there was not an attempt to open the lid before the unit came to a complete stop, see suggestions for the centrifuge not starting and giving an “ERROR: 7.1” error.</p> <p>If someone attempted to open the lid during the run cycle, please wait until the unit has come to a complete stop before opening the lid. Manually releasing the lid during the cycle creates a hazardous condition and is an OSHA safety violation.</p>
	ERROR: 7.3 - Indicates the lid safety interlock switch failed during deceleration or an attempt was made to open the lid before the unit came to a complete stop.	<p>If there was not an attempt to open the lid before the unit came to a complete stop, see suggestions for the centrifuge not starting and giving an “ERROR: 7.1” error.</p> <p>If someone attempted to open the lid during the run cycle, please wait until the unit has come to a complete stop before opening the lid. Manually releasing the lid during the cycle creates a hazardous condition and is an OSHA safety violation.</p>
	ERROR: 8 - Indicates the speed was too erratic.	Check electrical outlet for stable line voltage, and ensure that the circuit isn’t overloaded.

Troubleshooting

SYMPTOM	The sample temperature is exceeding 39°C.	
	POSSIBLE CAUSES	POSSIBLE SOLUTIONS
	The rotor chamber heat extraction fan isn't turning on.	Verify that the fan is turning on when the cycle is started, continues to run during the cycle, and for several minutes after the rotor comes to a complete stop.
	Cycle times are too long, operating speed is too high, and /or cycles are too frequent.	Lower the operating speed (see Appendix B R.C.F. Chart for appropriate speed), shorten spin time, and/or allow more cooling time between cycles with the lid open.
	Centrifuge is under a heat vent.	Relocate the centrifuge away from heat vents.
Centrifuge's immediate ambient environment is warm due to other equipment.	Relocate unit away from heat producing equipment.	

Chapter 6

Limited Warranty Statement

New Silencer[®] centrifuges are warranted to be free from defects in material and workmanship for a period of one year from the date of delivery. GFMD, Ltd., or its agent, will repair or replace and return free of charge any part that is returned, transportation prepaid by user, to GFMD, Ltd., or its agent, within said period, and that is found upon inspection to have been defective in materials or workmanship.

There is an additional one year warranty on parts plus an additional three years on the motor. During this period GFMD, Ltd., or its agent, will repair or replace and return free of charge any part that is returned, transportation prepaid by user, to GFMD, Ltd., or its agent, within said period, and that is found upon inspection to have been defective in materials or workmanship. Labor is not included during this period.

These warranties do not include normal wear from use, or operator maintenance. It does not apply to any instrument or part that has been altered by anyone other than an employee of the manufacturer or its agent nor to any instrument that has been damaged through accident, negligence, failure to follow operating instructions, natural disaster, the use of electric currents of circuits other than those specified on the plate affixed to the instrument, insufficient or excessive electrical supply, operation on emergency or backup generators, abnormal mechanical or environmental conditions, misuse or abuse.

GFMD, Ltd. reserves the right to change, alter, modify or improve any of its instruments without any obligation whatsoever to make corresponding changes to any instrument previously sold or shipped.

The foregoing obligations are in lieu of all other obligations including negligence and all warranties of merchantability or otherwise, expressed or implied in fact or by law and state our entire and exclusive liability and buyer's exclusive remedy for any claim or damages in connection with the sale or furnishing of goods or parts, their design, suitability for use, installation or operation. GFMD, Ltd., or its agent, will in no event be liable for any special or consequential damages whatsoever, and our liability under no circumstances will exceed the contract price for the goods for that liability is claimed.

Appendix A

Specifications

PERFORMANCE SPECIFICATIONS

- Maximum speed:
 - S2410SP w/ 8 x 10ml Horizontal Rotor 4,500 RPM
 - S2410SP-HZ2 w/ 12 x 10ml Horizontal Rotor 4,500 RPM
 - S2410SP-LV w/ 10 x 10ml FA Rotor 5,000 RPM
 - S2410SP-HS w/ 6 x 10ml Horizontal Rotor 5,500 RPM
 - S2410SP-PPP w/ 12 x 5ml FA Rotor 6,000 RPM
 - S2410SP-SC w/ 8 x 5ml FA Rotor 6,000 RPM

- Maximum RCF:
 - S2410SP w/ 8 x 10ml Horizontal Rotor 3,060 x g
 - S2410SP-HZ2 w/ 12 x 10ml Horizontal Rotor 3,060 x g
 - S2410SP-LV w/ 10 x 10ml FA Rotor 3,460 x g
 - S2410SP-HS w/ 6 x 10ml Horizontal Rotor 4,500 x g
 - S2410SP-PPP w/ 12 x 5ml FA Rotor 3,847 x g
 - S2410SP-SC w/ 8 x 5ml FA Rotor 4,039 x g

- Approximate acceleration rate (0 - Max. RPM): 10 seconds

- Approximate deceleration rate (Max. - 0 RPM):
 - S2410SP w/ 8 x 10ml Horizontal Rotor 25 seconds
 - S2410SP-HZ2 w/ 12 x 10ml Horizontal Rotor 25 seconds
 - S2410SP-LV w/ 10 x 10ml FA Rotor 60 seconds
 - S2410SP-HS w/ 6 x 10ml Horizontal Rotor 30 seconds
 - S2410SP-PPP w/ 12 x 5ml FA Rotor 60 seconds
 - S2410SP-SC w/ 8 x 5ml FA Rotor 60 seconds

- Maximum noise level: 58 dBA

- Speed Control +/- 2%

- Timer +/- 5%

- Power requirements: 115 volts, 5 amperes

UNIT SPECIFICATIONS

- Dimensions 13”w x 16.5”d x 11.5”h
- Spill resistant control panel
- Completely enclosed rotor chamber
- High-strength alloy rotor chamber
- See-through high-strength lid
- Dual safety interlock to ensure lid is closed and locked
- Direct drive system
- Brushless D.C. motor (2/3 HP)
- Microprocessor control
- Digital speed display
- Digital R.C.F. display
- Digital time display
- Timer range 1 - 999 plus hold

Appendix B

R.C.F. Chart

RELATIVE CENTRIFUGAL FORCE CHART								
RPM	R.C.F.							
	S2410SP and S2410SP-HZ2		S2410SP-LV		S2410SP-HS		S2410SP-PPP	S2410SP-SC
		w/ 5ml Adapter		w/ 5ml Adapter		w/ 5ml Adapter		
500	38	32	35	30	37	31	27	28
600	54	46	50	43	54	45	38	40
700	74	63	68	59	73	62	52	55
800	97	82	89	77	95	80	68	72
900	122	104	112	98	120	102	87	91
1,000	151	128	138	121	149	126	107	112
1,100	183	155	167	146	180	152	129	136
1,200	218	185	199	174	214	181	154	162
1,300	255	217	234	204	251	212	181	190
1,400	296	252	271	237	292	246	209	220
1,500	340	289	311	272	335	283	240	252
1,600	387	329	354	309	381	322	274	287
1,700	437	371	400	349	430	363	309	324
1,800	490	416	448	391	482	407	346	363
1,900	546	464	500	436	537	454	386	405
2,000	605	514	554	483	595	503	427	449
2,100	666	566	610	532	656	555	471	495
2,200	731	621	670	584	720	609	517	543
2,300	799	679	732	638	787	665	565	593
2,400	870	740	797	695	857	724	616	646
2,500	945	803	865	754	930	786	668	701
2,600	1,022	868	935	816	1,006	850	722	758
2,700	1,102	936	1,009	880	1,084	917	779	818
2,800	1,185	1,007	1,085	946	1,166	986	838	880
2,900	1,271	1,080	1,164	1,015	1,251	1,057	899	943
3,000	1,360	1,156	1,245	1,086	1,339	1,132	962	1,010

RELATIVE CENTRIFUGAL FORCE CHART

RPM	R.C.F.							
	S2410SP and S2410SP-HZ2		S2410SP-LV		S2410SP-HS		S2410SP-PPP	S2410SP-SC
		w/ 5ml Adapter		w/ 5ml Adapter		w/ 5ml Adapter		
3,100	1,452	1,234	1,330	1,160	1,430	1,208	1,027	1,078
3,200	1,548	1,315	1,417	1,236	1,523	1,288	1,094	1,149
3,300	1,646	1,398	1,507	1,314	1,620	1,369	1,164	1,222
3,400	1,747	1,484	1,600	1,395	1,720	1,454	1,235	1,297
3,500	1,851	1,573	1,695	1,478	1,822	1,540	1,309	1,374
3,600	1,959	1,664	1,793	1,564	1,928	1,630	1,385	1,454
3,700	2,069	1,758	1,894	1,652	2,037	1,721	1,463	1,536
3,800	2,182	1,854	1,998	1,743	2,148	1,816	1,543	1,620
3,900	2,299	1,953	2,105	1,835	2,263	1,912	1,626	1,706
4,000	2,418	2,054	2,214	1,931	2,380	2,012	1,710	1,795
4,100	2,540	2,158	2,326	2,029	2,501	2,114	1,797	1,886
4,200	2,666	2,265	2,441	2,129	2,624	2,218	1,885	1,979
4,300	2,794	2,374	2,559	2,231	2,751	2,325	1,976	2,074
4,400	2,926	2,486	2,679	2,336	2,880	2,434	2,069	2,172
4,500	3,060	2,600	2,802	2,444	3,012	2,546	2,164	2,272
4,600			2,928	2,553	3,148	2,661	2,261	2,374
4,700			3,057	2,666	3,286	2,778	2,361	2,478
4,800			3,188	2,780	3,427	2,897	2,462	2,585
4,900			3,323	2,897	3,572	3,019	2,566	2,694
5,000			3,460	3,017	3,719	3,143	2,672	2,805
5,100					3,869	3,270	2,780	2,918
5,200					4,022	3,400	2,890	3,033
5,300					4,179	3,532	3,002	3,151
5,400					4,338	3,667	3,116	3,271
5,500					4,500	3,804	3,233	3,394
5,600							3,352	3,518
5,700							3,472	3,645
5,800							3,595	3,774
5,900							3,720	3,905
6,000							3,847	4,039

Service Log

Service Log		
Date	Service Performed	By

Appendix D

Replacement Parts List

Description	Qty Needed	Part No.
Gasket, Lid	1 ea.	SIL00476
Gasket, Motor, S2410SP-PPP / SP-SC	1 ea.	SIL00456A
Gasket, Motor, S2410SP / SP-LV / SP-HS	1 ea.	SIL00456B
Hinge, Lid, S2410 v2	2 ea.	SIL00512
Latch, Lidlock	1 ea.	SIL00642B
Lid, S2410 v2	1 ea.	SIL00661
Lidlock Assembly	1 ea.	SIL00671B
Solenoid (part of SIL00671B)	1 ea.	SIL00131
Switch, Lid Interlock (part of SIL00671B)	1 ea.	SIL02456
Switch, Lock Interlock (part of SIL00671B)	1 ea.	SIL02457
Motor Assembly, S2410SP / SP-LV / SP-HS	1 ea.	SIL00730A
Motor Assembly, S2410SP-PPP / SP-SC	1 ea.	SIL00730C
Mounting Bracket, Motor	2 ea.	SIL00787
Nut, Rotor Securing	1 ea.	SIL00791
P.C.B., Display / Control, SP	1 ea.	SIL00815A
P.C.B., Power, S2410 / S2450E	1 ea.	SIL00841

Parts are sold individually. The quantity listed is the quantity used per unit.

Lid Release Tool

 **WARNING**

The lid release tool is provided for emergency access to samples only. Unplug the centrifuge before attempting this procedure!

The correct tool must be used for your unit or the lid safety interlock switch may become damaged. If the interlock switch is damaged the unit can't detect the lid being closed and therefore won't start.

To use the release tool:

1. Unplug the centrifuge.
2. Insert the tool completely into the release access port on the left side of the unit (just below the lid locking bracket).
3. Push the handle towards the back of the unit and lift the centrifuge lid.